

S & N LABS

2021 E. Fourth Street

Santa Ana, California 92705

(714) 543-2211

16 August 2020

Job Number:	23734d
PO Number:	verbal

Quality Control
advancedresearch.bio
601 QC-132
Sorel-Tracy, QC, Canada J3R 1K9

REPORT OF ANALYSIS

One amber jar labeled "MK2866-arc" was received on 16 August 2020. The powder in the jar was analyzed for identification using Fourier-transform infrared spectroscopy (FT-IR). The resulting spectrum matched a reference sample of this material.

The material was also analyzed for purity using high pressure liquid chromatography (HPLC). The detector was set to 210nm. The results are summarized in the table below.

Sample	Chromatographic Purity (% area)
MK2866-arc	>98.9

The spectrum and chromatogram are enclosed for your reference.

Neil E. Spingarn, Ph.D.
President

3690

S&N Labs

2021 E. Fourth Street, Suite 112
Santa Ana, CA 92705
Tel: 714-543-2211


Sample: MK2866-arc

Date: 08/16/2020

Analyst: Marcus Lamont

Client:

advancedresearch.bio

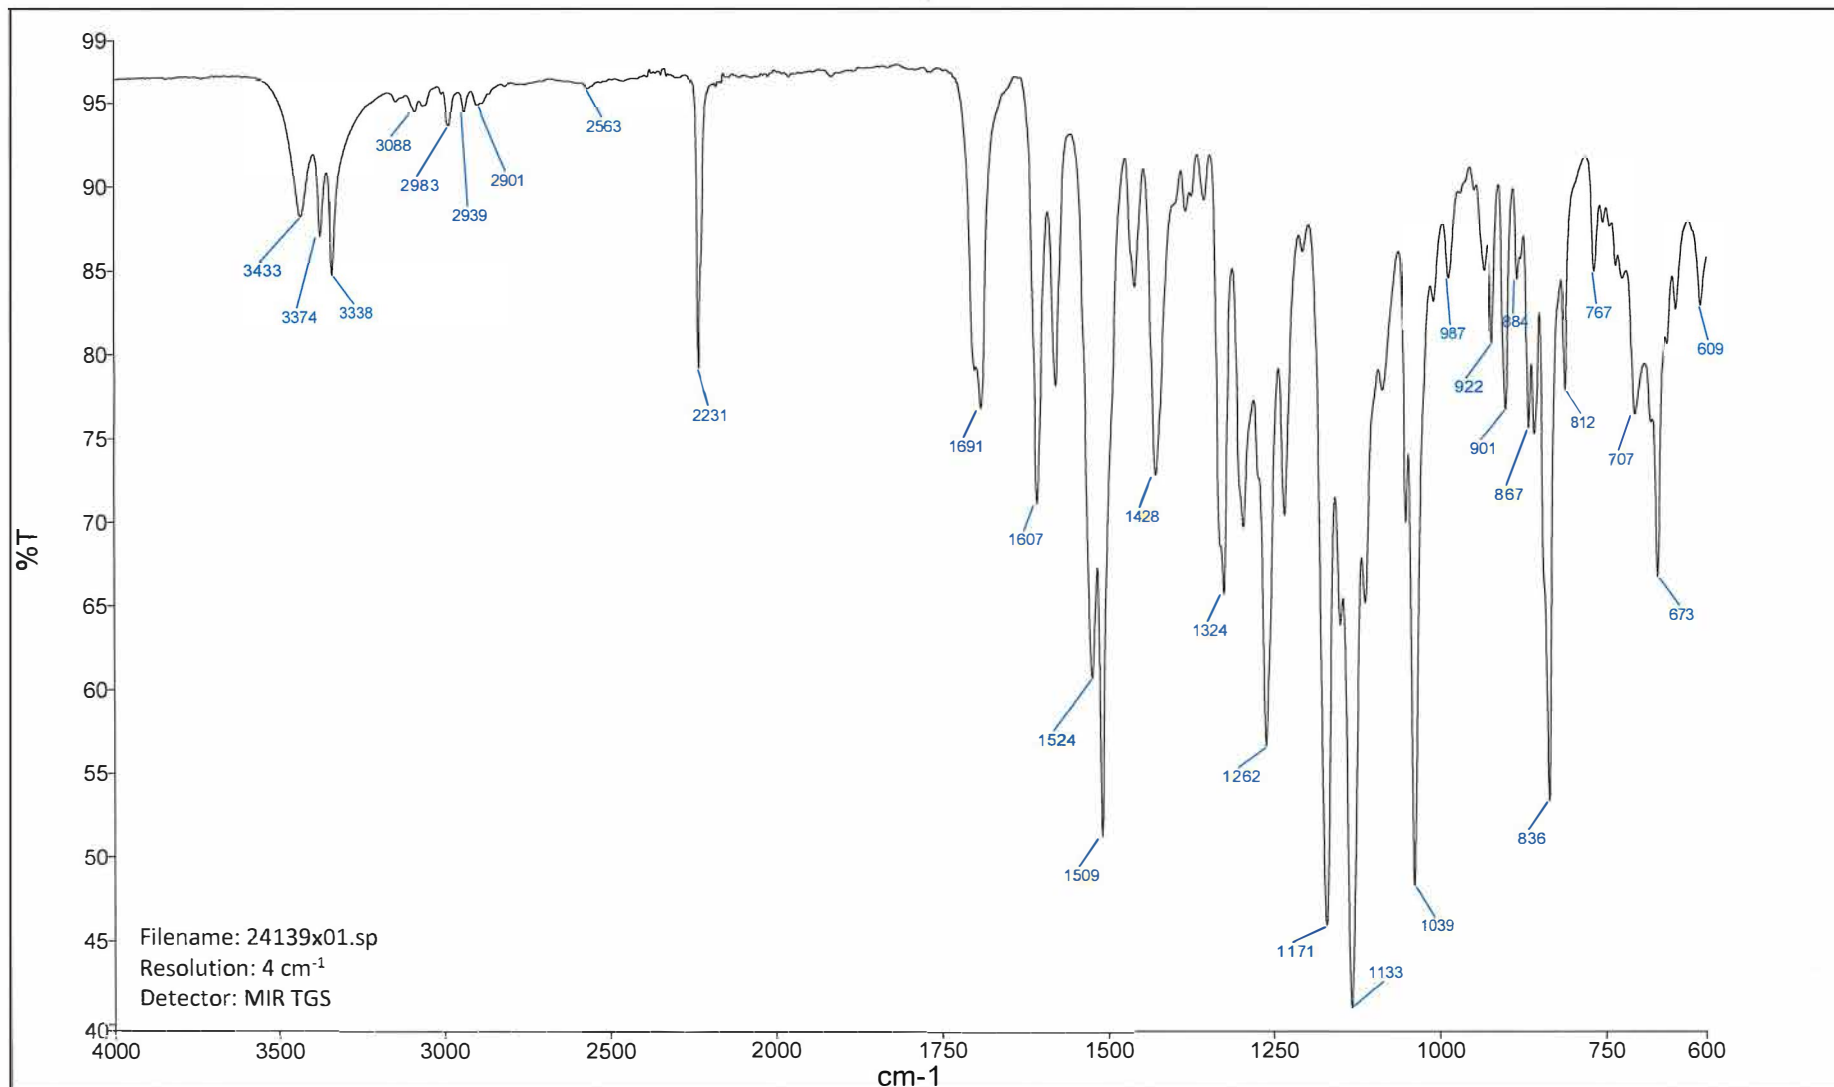


Chromatogram and Results

Injection Details

Injection Name:	MK2866-arc; 20ppm A3	Run Time (min):	20.00
Vial Number:	Unknown	Injection Volume:	10.00
Injection Type:		Channel:	UV_VIS_1
Calibration Level:	BD 150mm Max RP	Wavelength:	210.0
Instrument Method:	Processing Method	Bandwidth:	5
Processing Method:	16/Aug/20 21:28	Dilution Factor:	1.0000
Injection Date/Time:		Sample Weight:	1.0000

Chromatogram

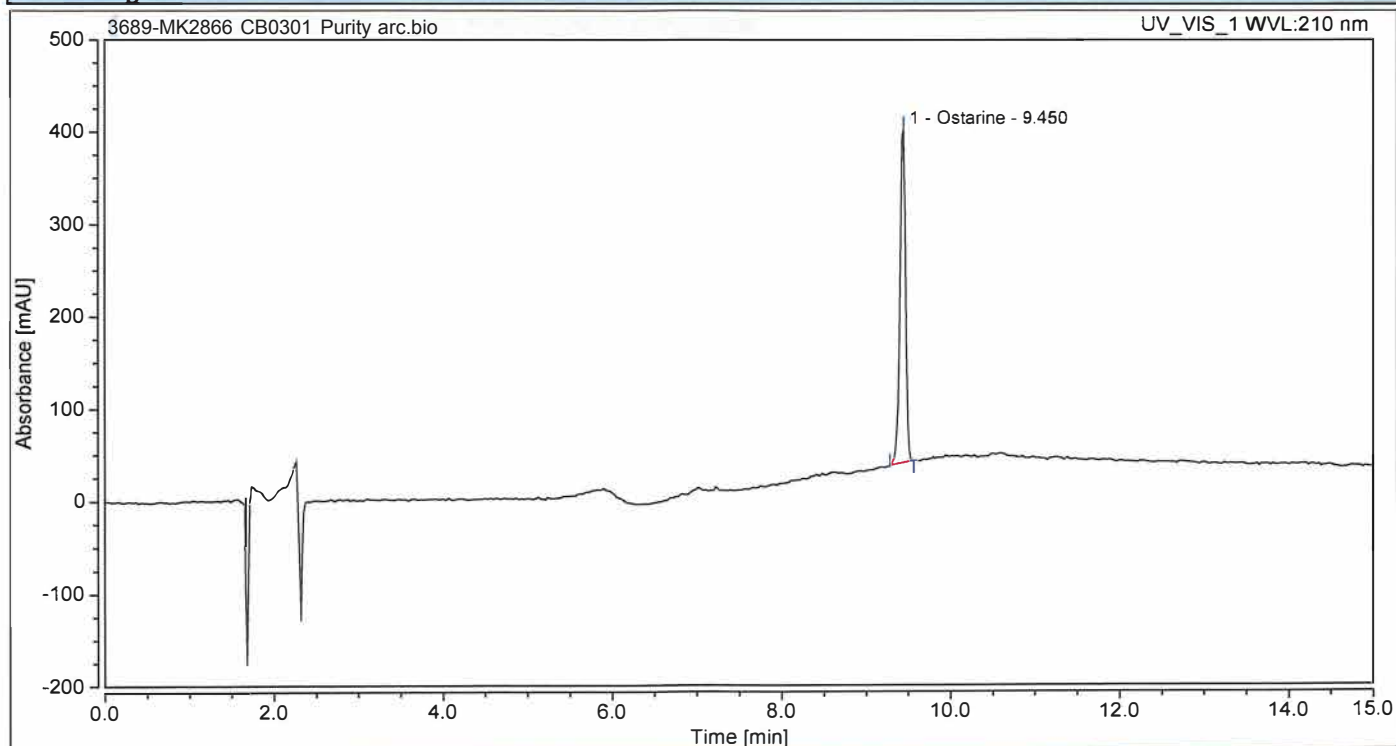

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount µg/ml
1	MK2866	9.450	28.196	361.627	98.9	98.9	n.a.
Total:			28.196	361.627	98.9	98.9	